

Fig. 1

0956350-09204

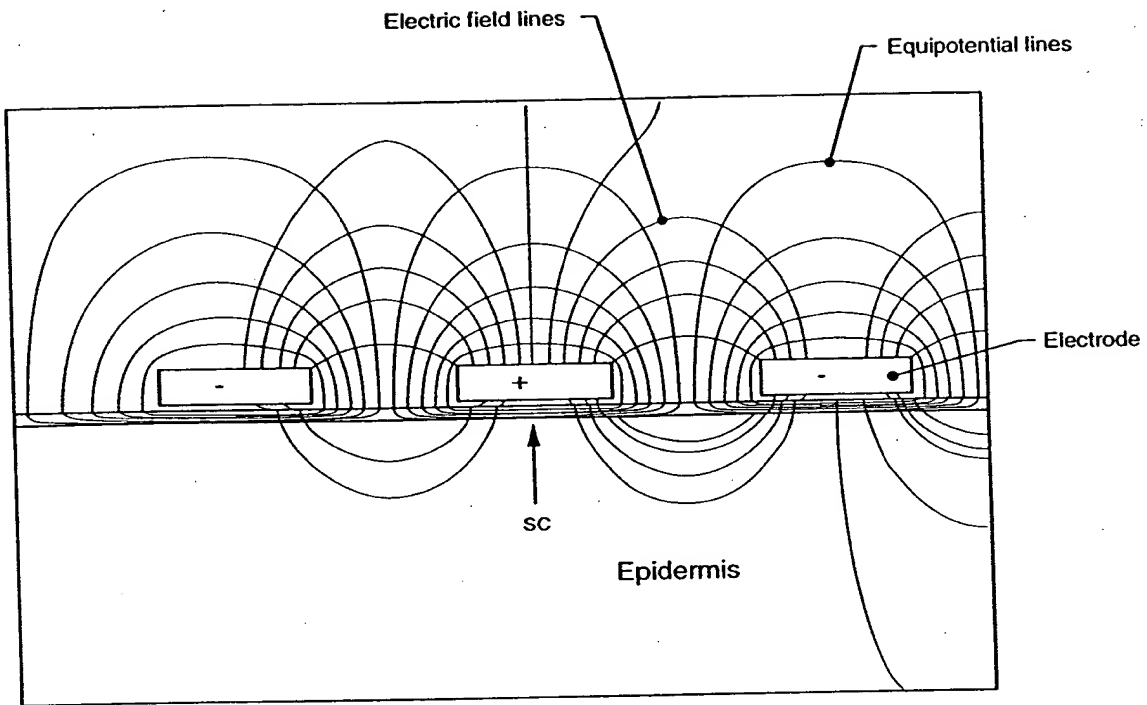


Fig. 2

0956350 092704  
T02260 0629560

# FIELD STRENGTH BELOW AN ELECTRODE BEFORE BREAKDOWN OF THE S.C.

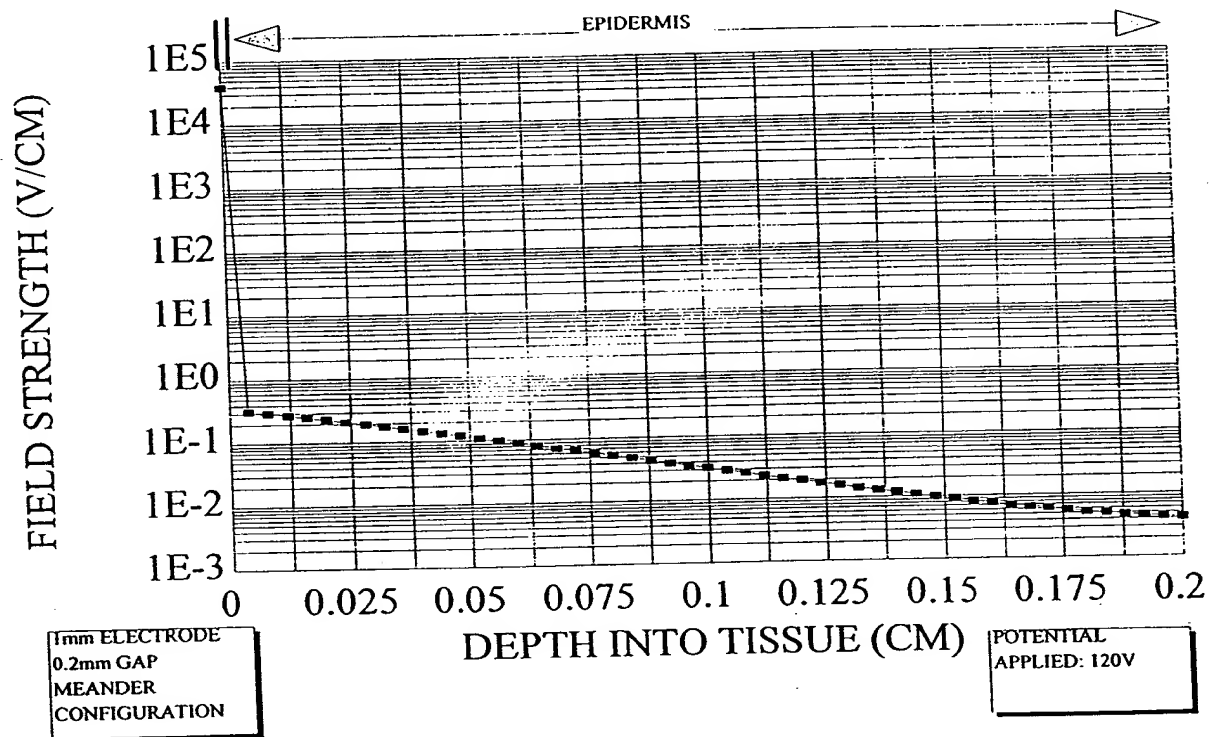


Fig. 3A

FOUO 060350

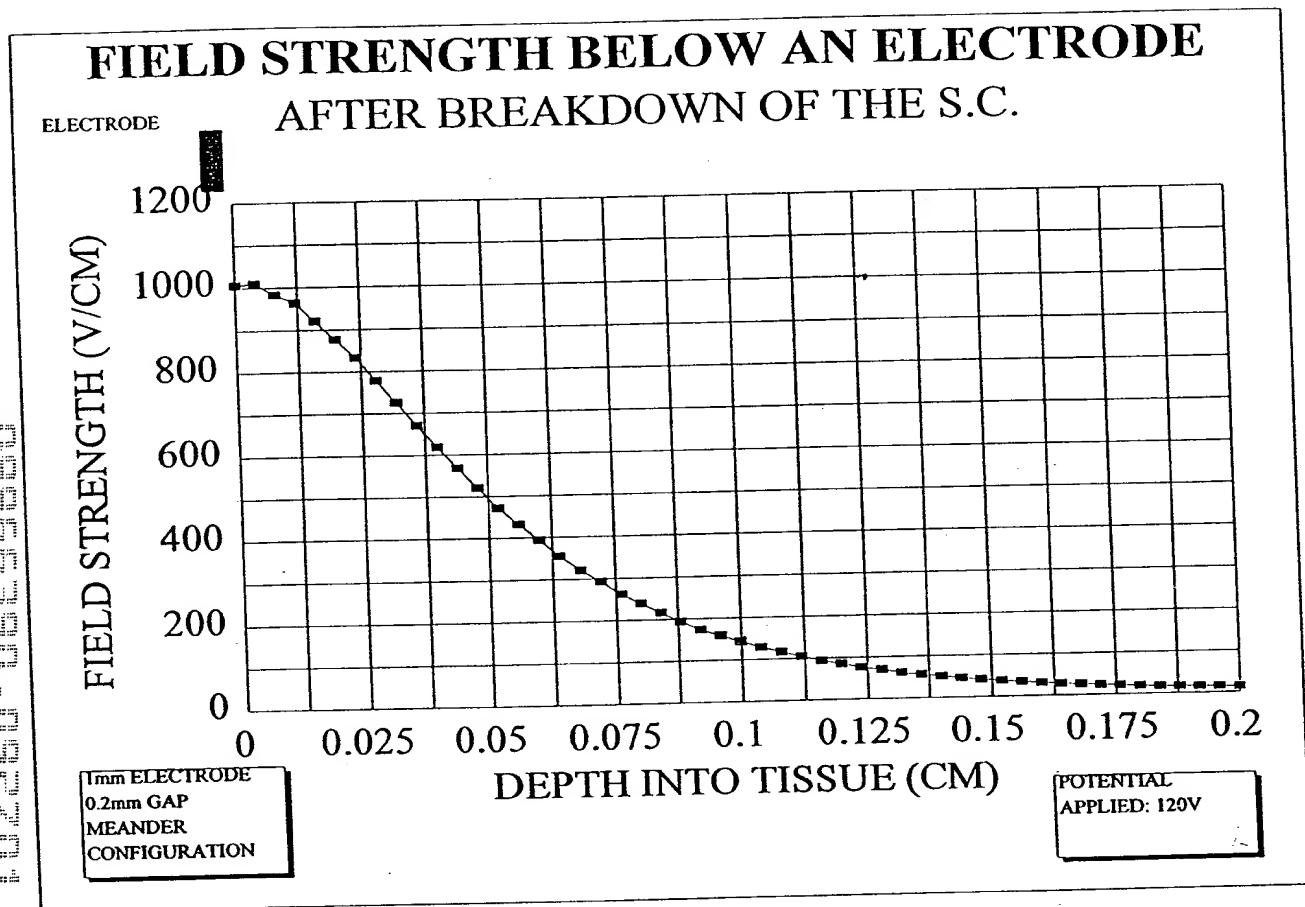


Fig. 3B


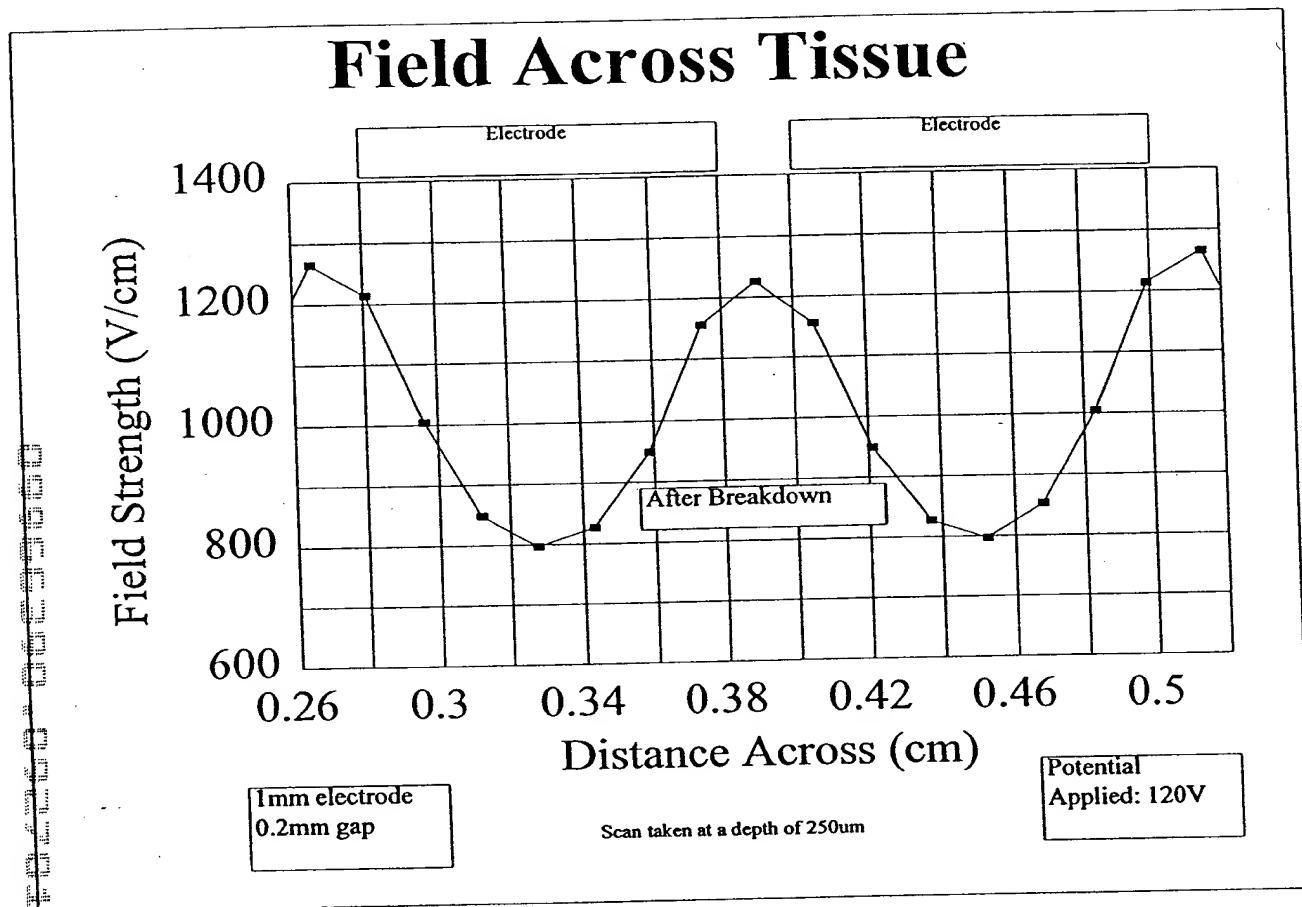


Fig. 4A

## Field Across Tissue

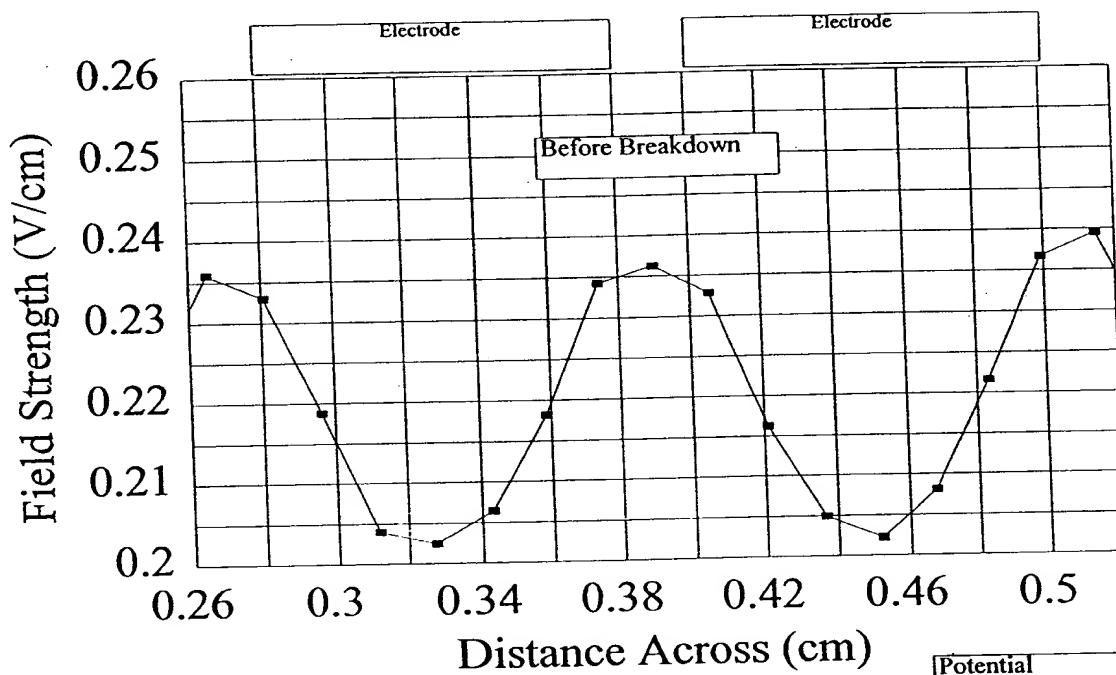

1mm electrode  
0.2mm gap

Scan taken at a depth of 250um

Potential  
Applied: 120V

Fig. 4B

702260 06E99660

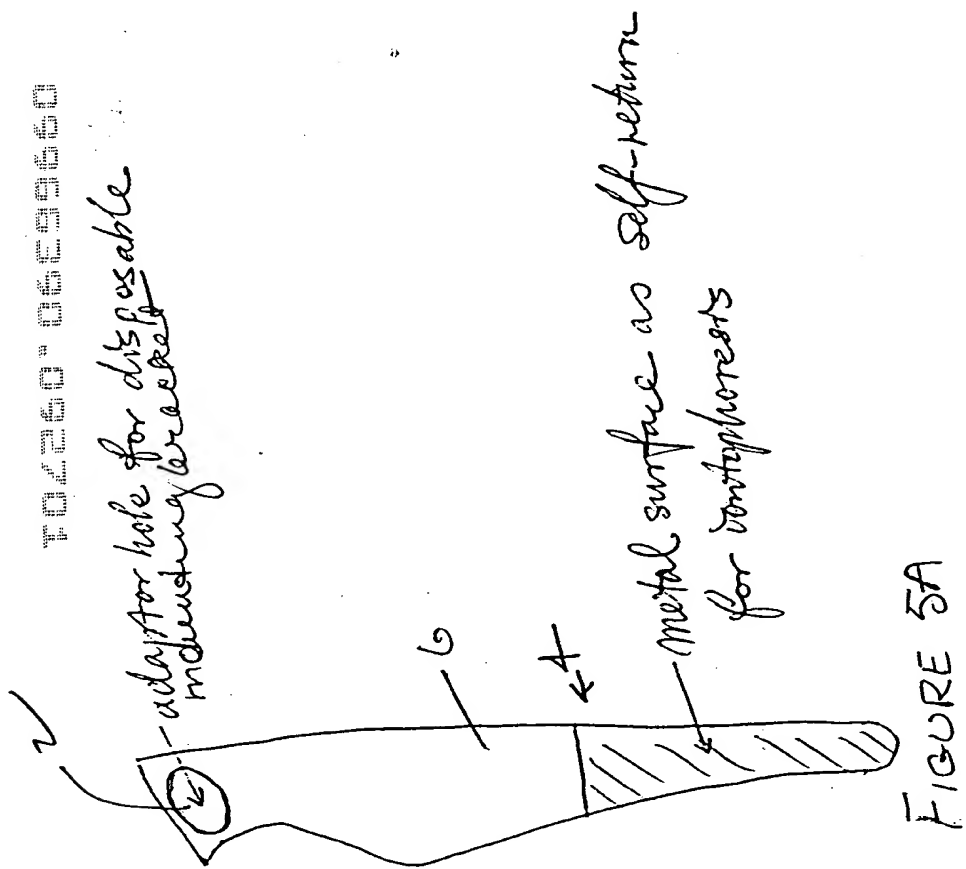


FIGURE 5A

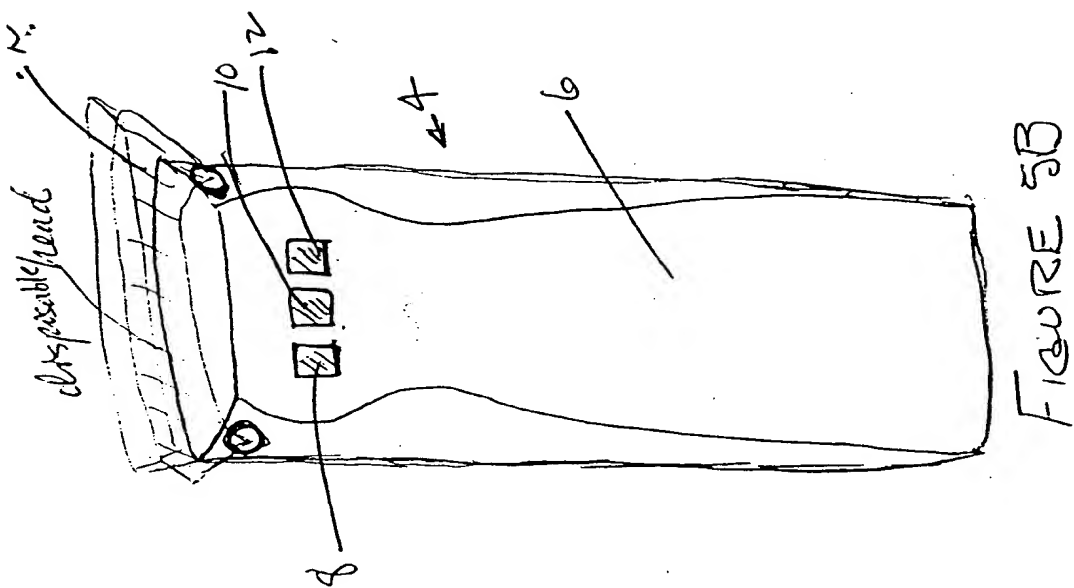


FIGURE 5B

Battery-powered hand held pulser  
FIGURES 5A-B

adaptor with disposable electrocosmetic felt.



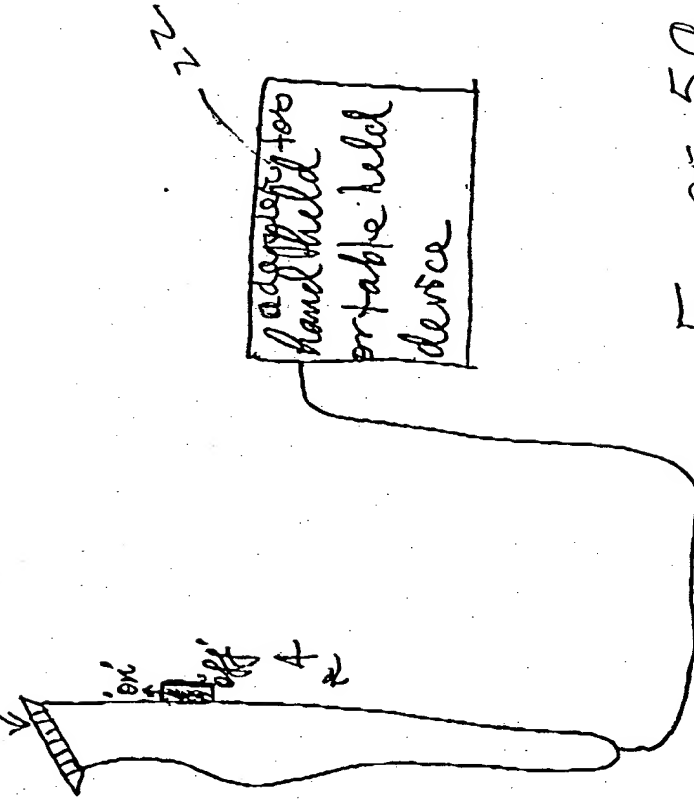



FIGURE 5C

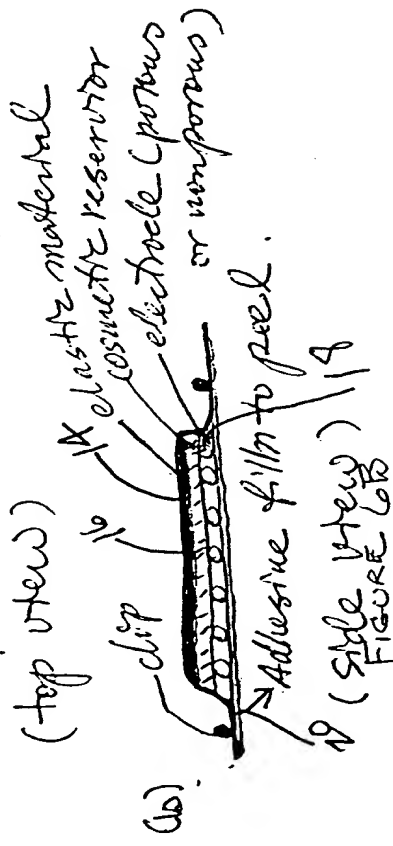

square type:

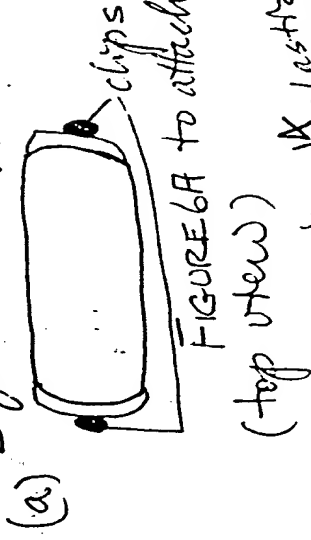


(c) moon type:

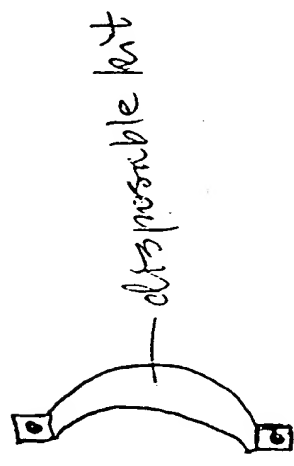

(top view)  
FIGURE 6C

round type

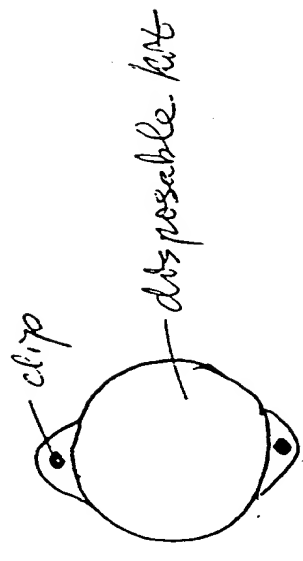

(top view)  
FIGURE 6D

(e) roller type  
sponge soaked with cosmetic prep.  
needle electrode


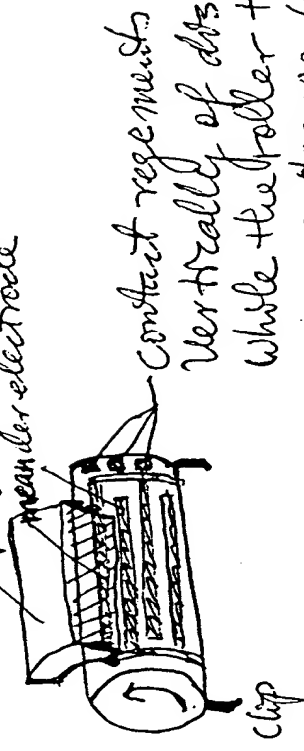


FIGURE 6E

FIGURES 6A-E  
Different Configurations of disposable mounting bracket  
(size can be smaller large)

TOP 260 06299550

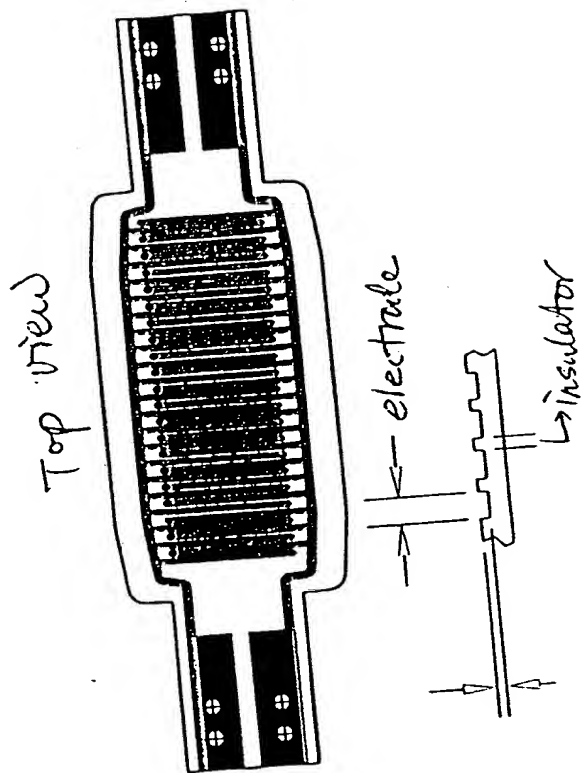

porous electrode  
FIGURE 7